

Automated Wheel Chair Using Multiple Methods In Android Technology

V. Gokula Krishnan, V. Divya

Abstract : The wide spread prevailing loss of limbs in everyday situation because of wars, mishaps, accidents, age and medical issues. The main aim of the project is to automate the Control of Wheelchair movements with all directions and producing the emergency alert as well. Elderly peoples can't walk; we have to deal with these peoples each day. Thus, we are utilizing the wheelchair for transporting these peoples. It is difficult for the incapacitated and elderly individuals to move a mechanical wheelchair, which huge numbers of them typically use for velocity. Subsequently there is a requirement for outlining a wheelchair that is clever and gives simple transportation to the physically-challenged peoples as well as elderly peoples. In this specific circumstance, an endeavor has been made to propose an idea controlled wheelchair, which utilizes the caught signals from the client's activity and procedures it to control the wheelchair. The triggers which are caught are converted into movement triggers by the microcontroller which thus moves the wheelchair. For all the entire system properly supports the elderly people to supplement their physical illness and provides a wonderful solution to live the independent life without other's physical needs for moving from one place to other place in respective places.

Index Terms: Electronic Wheel Chair, Healthcare, Transportation.

1. INTRODUCTION

As of late as the silver age has been exponentially expanding, the social requests about the personal satisfaction likewise have been expanding relatively to them. Numerous mechanical specialists have been attempting to consolidate the apply autonomy ability into the welfare frameworks for the impaired and the elderly. Since a guide robot for the visually impaired was first introduced, there are numerous looks into about such guide robot^{2, 3, 4} and many more. A wheelchair robot for versatility helps for the disabled is likewise introduced. Since the design of the wheelchair robot is like the portable robot, numerous victories were introduced. Such looks into have been focused on detecting and way arranging since confinement and snag evasion are vital issues in the portable apply autonomy.

2 LITERATURE SURVEY

In 2014, the authors R.R.J.P.D.H.J. Pandya and Hyun Tae Kim [1] proposed manufacture and portrayal of a minimal effort MEMS based piezo-resistive smaller scale drive sensor with SU-8 tip utilizing research facility made silicon-on-protector (SOI) substrate. To plan SOI wafer, silicon film (0.8 μm thick) was stored on an oxidized silicon wafer utilizing RF magnetron sputtering procedure. The micro cantilever drive sensor was incorporated with an electronic module that distinguishes the adjustment in protection of the sensor concerning the connected power and shows it on the PC screen. In 2009, Y.J. Li, J. Zhang, Z.Y. Jia, M. Qian, and H. Li [3] described a novel piezoelectric six-part drive/torque sensor with four-point supporting structure, and makes look into on constrain detecting component's spatial game plan of the novel sensor. Two sorts of various spatial plans are propelled, tablet and square course of action. The numerical models are constructed and figured. Keeping in mind the end goal to

examine the legitimacy of the proposed strategy, a model of piezoelectric six-segment compel/minute sensor is created with two sorts of various spatial courses of action, and trademark trial of the piezoelectric six-part constrain/minute sensor are performed. In the year of 2014, Y. Tenzer, L.P. Jentoft, and R.D. Howe [12] proposed a framework which introduces another way to deal with the development of material exhibit sensors in view of barometric weight sensor chips and standard printed circuit sheets (PCBs).. The subsequent exhibit hardware can be effortlessly exemplified with delicate polymers to give strong and agreeable getting a handle on surfaces for particular hand outlines. This approach guarantees to make delicate, powerful, and modest material detecting accessible for an extensive variety of mechanical technology and human-interface applications.

3 PAST SYSTEM ANALYSIS

In existing system, there is automated way to operate a wheel chair. So the wheel chair can be operated with own hand or with someone's help. So, handless people felt very difficult to operate it. To overcome these problems we go for proposed system.

The existing wheelchairs have some disadvantages and some of them are listed below: (i) The wheel chair robot is difficult to operate (ii) There is no alternative method is used to operate the wheel chair in this system (iii) Low in Performance, requires heavy manual operations to perform (iv) Cost Expensive in nature and (v) Modes of control is limited, only higher end models contains some interesting features, but it is too costly to purchase.

4 PROPOSED SYSTEM SUMMARY

In our project, we are introducing advanced method to control the wheel chair with the help of embedded systems. Here we are introducing two methods for controlling the wheel chair. (a) Hand gesture control (b) smart phone control. Here robot can be operated in four ways like forward, reverse, left and right with the hand Gesture signal movement. But some cases hand gesture is not possible to operate a wheel chair. Therefore we introduce alternate way to operate a wheel chair with the help of android mobile. Using this android application, it can be used with 3 in 1 option. We can control the wheelchair robot with three methods using this application.

- V. Gokula Krishnan is currently pursuing PhD in Computer Science and Engineering in Sathyabama Institute of Science and Technology, Chennai and also working as Associate Professor in the Department of CES in Panimalar Institute of Technology, Chennai. E-mail: gokul.kris143@yahoo.com
- V. Divya is currently pursuing PhD in Electrical and Electronics Engineering in Sathyabama Institute of Science and Technology, Chennai. E-mail: vdivya6891@gmail.com

There are Steering control, Voice control, and touch screen button control. Also Ultrasonic sensor is used to detect the obstacle. LCD is used to display the various statuses. The wheel chair can also be operated automatically using a pre-defined path. The proposed wheelchair model has lots of advantages and some of them are listed below: (i) this method is easy to operate the wheel chair. (ii) In addition of voice is used to control the wheel chair. (iii) For a safety monitoring of ultrasonic sensor is used.

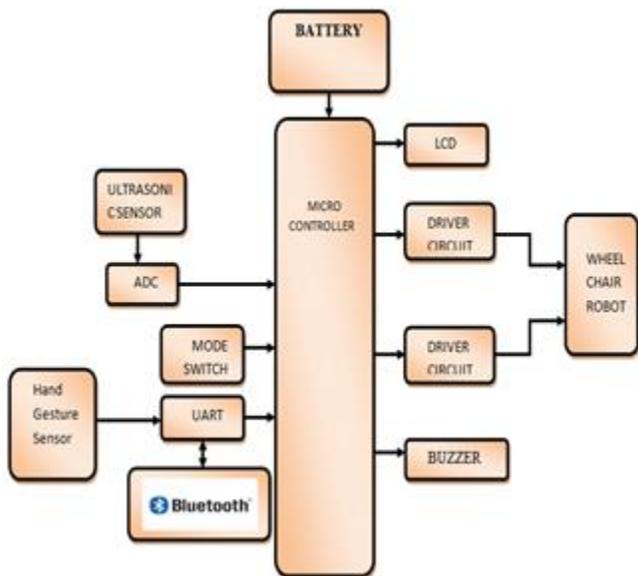


Fig.1 Proposed System Architecture

However the real client of the wheelchair robot is the impaired, so the wheelchair robot must ensure the wellbeing and dependability while thinking about the client's goal. In like manner, late investigations embraced a human-robot interface in order to bring a human into the robot criticism control circle. We can see that a bio-flag, for example, the electromyogram (EMG) and human movement, for example, look bearing and facial direction were used as the interface technique. The incapacitated and the elderly are not ordinary physically, so the client's order might be erroneous. What's more, the tangible data got by outside sensors, for example, vision, sonar, and laser go discoverer likewise incorporates vulnerability. In these reasons, the security is the most extensive issue in the welfare mechanical technology.

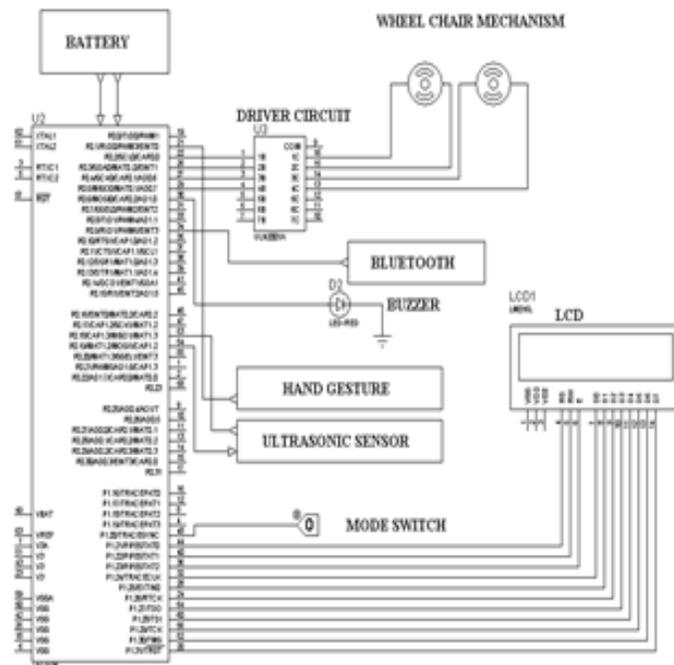


Fig.2 Circuit Diagram of the Proposed System

5 HAND GESTURE SUMMARY

Gesture recognition empowers people to speak with the machine and connect normally with no mechanical gadgets. Utilizing the idea of Gesture recognition, it is conceivable to point a finger at the PC screen so the cursor will move likewise. Motion location uses four directional photodiodes to detect reflected IR vitality to change over physical movement data to computerized data. The Gesture motor suits an extensive variety of cell phone motioning prerequisites: straightforward UP-DOWN-RIGHT-LEFT motions or more mind boggling motions can be precisely detected. Motion recognition, closeness identification, and RGB shading sense/surrounding light sense usefulness is controlled by a state machine, which reconfigures on-chip simple assets when each useful motor is entered. Each utilitarian motor contains controls like pick up, ADC incorporation time, hold up time, perseverance and edges that administer the activity. The control of the drove drive stick, LDR, is shared amongst vicinity and Gesture usefulness. The shading/ALS motor does not utilize the IR LED, but rather cross talk from IR LED discharges amid an optical example transmission may influence comes about.



Fig.3 Gesturing Device

6 ALGORITHM PROCEDURE

- Step-1: The system consists of mode switch to select different modes of operation.
- Step-2: Based on the mode selected, the gesture or voice based chair control is done.
- Step-3: The hand gesture module is used to drive the robot using hand gesture signal.
- Step-4: The ultrasonic sensor detects the distance between the person and the obstacle and reports it to controller.
- Step-5: Based on obstacle the wheel chair is driven in such a way it doesn't collide.
- Step-6: The user transmits a voice signal to mobile to drive the wheel chair
- Step-7: The signal is provided to the Bluetooth receiver and the respective motor is driven.

7 EXPERIMENTAL RESULTS

The following figure (Fig.4) illustrates the simulation view of the wheelchair design.

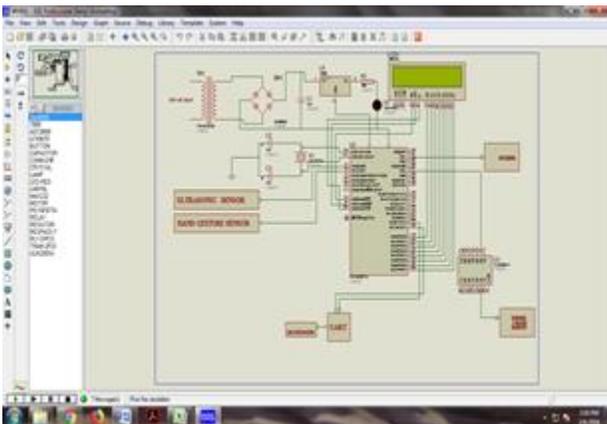


Fig.4 Simulation Model

The following figure (Fig.5) illustrates the hardware design view of the wheelchair design.

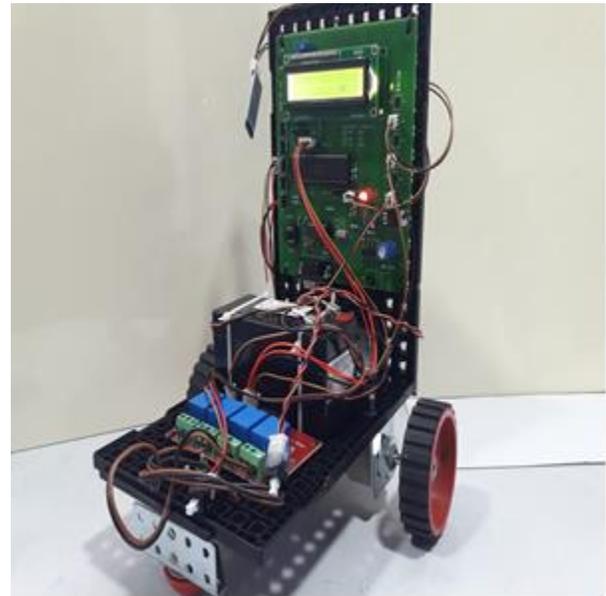


Fig.5 Wheelchair Design

8 CONCLUSION

The system eliminates the dependency of human for the disabled people to navigate them. The user can operate the chair using both hand gesture and voice signal. This helps for multiple disabled people of certain kind to use this system. Thus the physically challenged people can operate their vehicle independently without any additional assistance. They are free to control the vehicle using Voice commands or Gesture board. Thus the motors can move freely based on the user direction.

9 REFERENCES

- [1] R.R.J.P.D.H.J. Pandya, Hyun Tae Kim, "Mems based low cost piezoresistive microcantilever force sensor and sensor module," *Materials Science in Semiconductor Processing*, vol. 19, pp. 163–173, 2014.
- [2] C.Kang, "Performance improvement of a 6-axis force-torque sensor via novel electronics and cross-shaped double-hole structure," *International Journal of Control and Automation Systems*, vol. 3, no. 3, p. 469, 2005.
- [3] Y.J.Li, J. Zhang, Z.-Y. Jia, M. Qian, and H. Li, "Research on force-sensing element's spatial arrangement of piezoelectric sixcomponent force/torque sensor," *Mechanical Systems and Signal Processing*, vol. 23, no. 8, pp. 2687 – 2698, 2009. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S0888327009001514>
- [4] A.F. Fernandez, F. Berghmans, B. Brichard, P. Mgret, M. Decrton, M. Blondel, and A. Delchambre, "Multi-component force sensor based on multiplexed fibre bragg grating strain sensors," *Measurement Science and Technology*, vol. 12, no. 7, p. 810, 2001. [Online]. Available: <http://stacks.iop.org/0957-0233/12/i=7/a=310>
- [5] Y.L. Park, S. C. Ryu, R. Black, K. Chau, B. Moslehi, and M. Cutkosky, "Exoskeletal force-sensing end-effectors with embedded optical fiberbragg- grating

- sensors,” *Robotics, IEEE Transactions on*, vol. 25, no. 6, pp. 1319–1331, 2009.
- [6] F. Beyeler, S. Muntwyler, and B. J. Nelson, “Design and calibration of a microfabricated 6-axis force-torque sensor for microrobotic applications,” in *Robotics and Automation, 2009. ICRA'09. IEEE International Conference on*. IEEE, 2009, pp. 520–525.
- [7] F. Beyeler, S. Muntwyler, and B. J. Nelson, “A six-axis mems force– torque sensor with micro-newton and nano-newtonmeter resolution,” *Microelectromechanical Systems, Journal of*, vol. 18, no. 2, pp. 433– 441, 2009.
- [8] P. Berkelman, L. Whitcomb, R. Taylor, and P. Jensen, “A miniature microsurgical instrument tip force sensor for enhanced force feedback during robot-assisted manipulation,” *Robotics and Automation, IEEE Transactions on*, vol. 19, no. 5, pp. 917–921, 2003.
- [9] J. Rijkers, “Design of a miniature low-budget torque sensor,” *Technical Report 015CE2008*, University of Twente, Tech. Rep., 2008.
- [10] G. Hirzinger, J. Bals, M. Otter, and J. Stelter, “The dlr-kuka success story: robotics research improves industrial robots,” *Robotics Automation Magazine, IEEE*, vol. 12, no. 3, pp. 16–23, 2005.
- [11] (2013) The spacemouse family of 3d interface devices. [Online]. Available: <http://www.3dconnexion.com/products>
- [12] Y. Tenzer, L. P. Jentoft, and R. D. Howe, “Inexpensive and easily customized tactile array sensors using mems barometers chips,” 2014. *Robotics Automation Magazine, IEEE*, vol. 21, no. 3, 2014.
- [13] C. Reeks, M. G. Carmichael, D. Liu, and K. J. Waldron, “Angled sensor configuration capable of measuring tri-axial forces for phri,” *International Conference on Robotics and Automation*, 2016.
- [14] A. Bicchi, J. K. Salisbury, and D. L. Brock, “Contact sensing from force measurements,” *The International Journal of Robotics Research*, vol. 12, no. 3, pp. 249–262, 1993.
- [15] (2014) Honey well Torque Sensors Product Range Guide. [Online]. Available: <http://sensing.honeywell.com/honeywell-test-measurementtorque-range-guide-008897-1en.pdf>.